




Why are the labels listed multiple times using the N-Dataset comparison in the Calibration Data Manager (CDM)?



25.03.2020 - 1 -

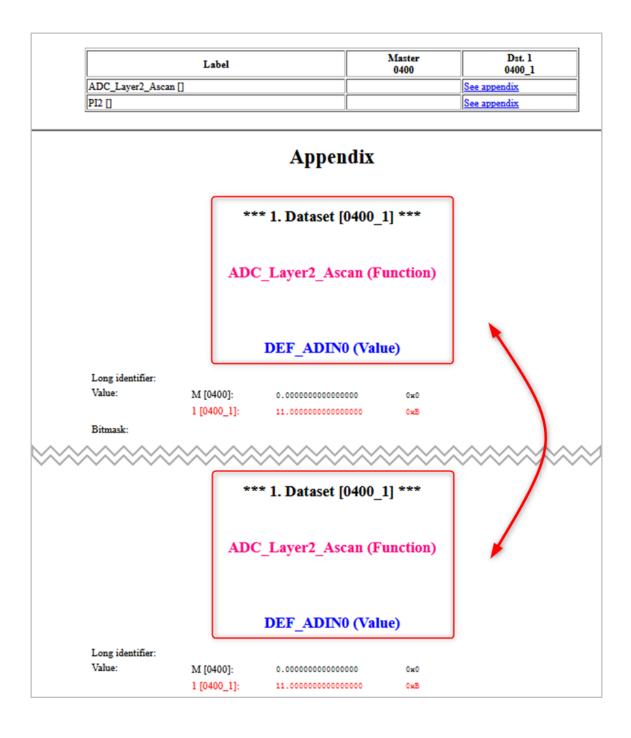





In an N-Dataset comparison, the labels are listed multiple times in the appendix for the following use case:

This behavior depends on the settings in the user options:

• The option "Group items by function" is set to "Flat function view":

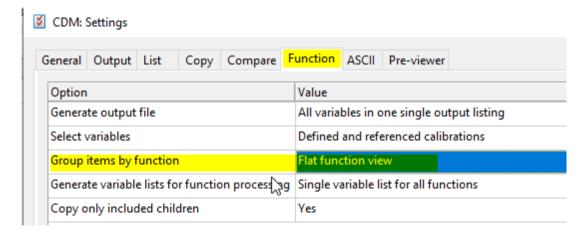

• "Output format for 2-dataset comparison" is set to "like N-dataset comparison":

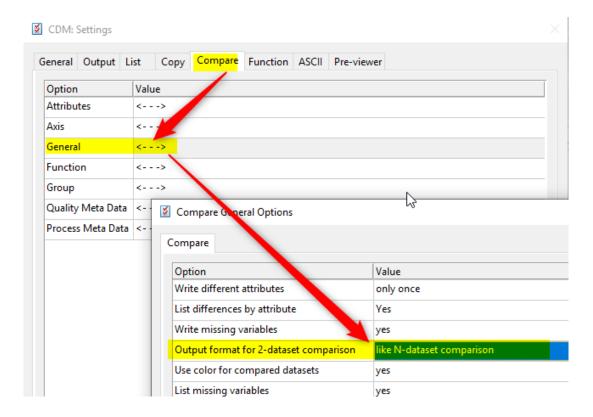


- 2 -



• "Sort appendix" is set to "dataset":




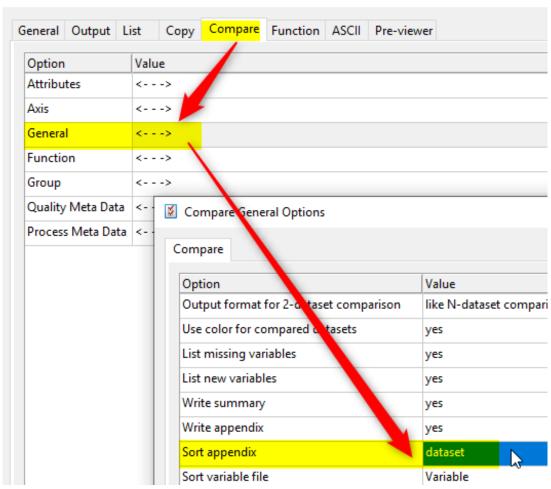



Solution: Set the option "Sort appendix" to "No"


CDM: Settings

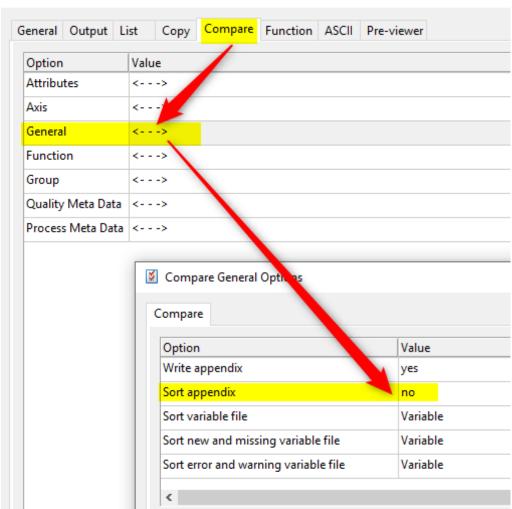



DRIVING EMBEDDED EXCELLENCE

The labels now are only listed once:

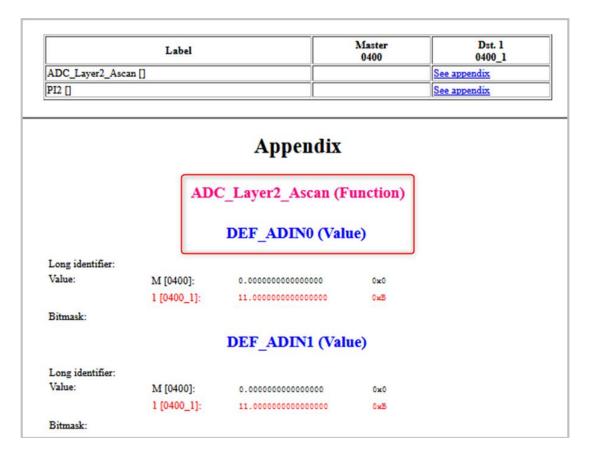



In case of further questions:

Please feel free to contact our Support Center, if you have further questions. Here you can find all information: http://www.etas.com/en/hotlines.php?langS=true&

This information (here referred to as "FAQ") is provided without any (express or implied) warranty, guarantee or commitment regarding completeness or accuracy. Except in cases of willful damage, ETAS shall not be liable for losses and damages which may occur or result from the use of this information (including indirect, special or consequential damages).